

FAULT FINDING

Should your Arctic bed fail to function, please check the following.

1. Check the Charger is plugged into a 13amp socket
2. Check to see if any of the following lights are showing on the charger.

Red - Charging

Amber - Charged

Green - Fully Charges

3. Check the connections of handset to the bed, the handset can be fitted to either the left or right hand side of the bed.
4. Ensure the bed frame is free of obstacles, ensuring all frames can lay flat to enable connections can be made.


Having checked the above, if the bed is still not functioning please contact

Centrobed on 01233 635353

Please could you ask for the Repairs Department

Arctic Handset Instructions

Each button has it's own function described below.

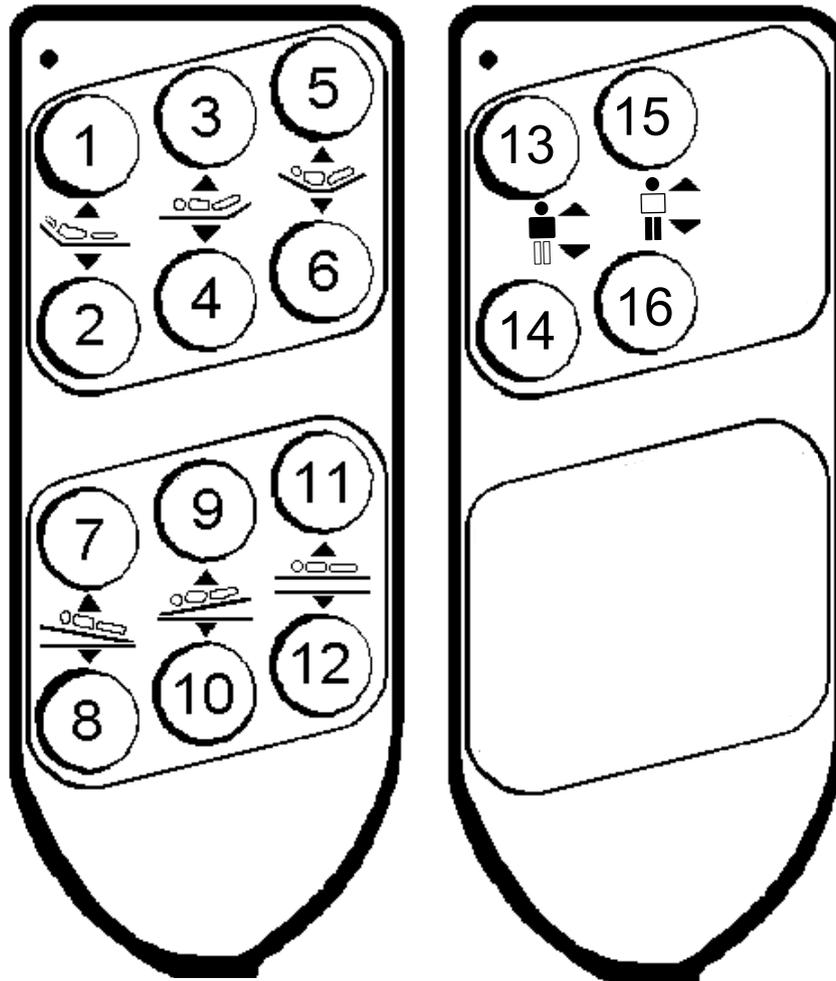

1. Raise to a sitting position
2. Lower from a sitting position
3. N/A
4. N/A
5. Positive Trendelenburg
6. Decrease Trendelenburg
7. Raise left side
8. Lower left side

9. Raise right side
10. Lower right side
11. Raise Bed
12. Lower bed
13. Left raise knee break
14. Left lower knee break
15. Right raise knee break
16. Right lower knee break